

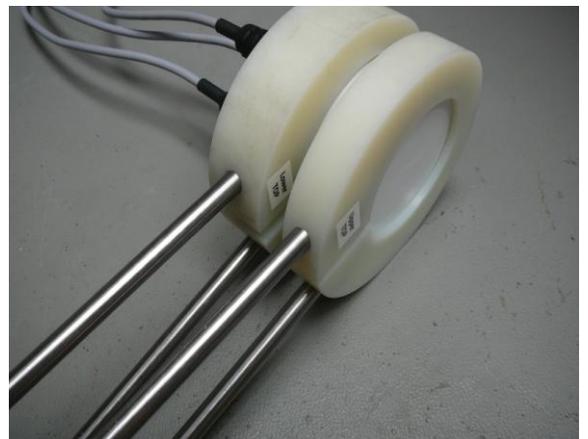


MicroLog ERi, SP3, V3, D3, T3

dataloggers – enclosure opening with a special tool

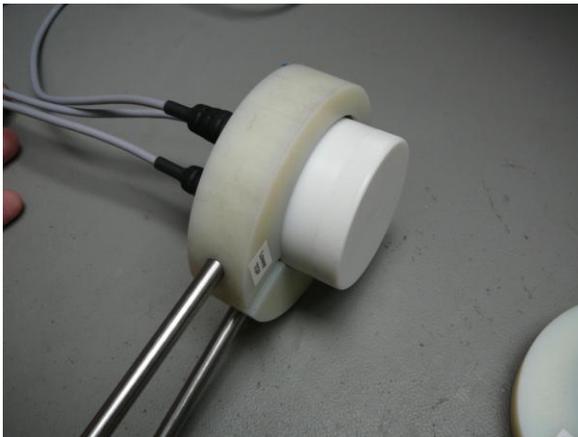

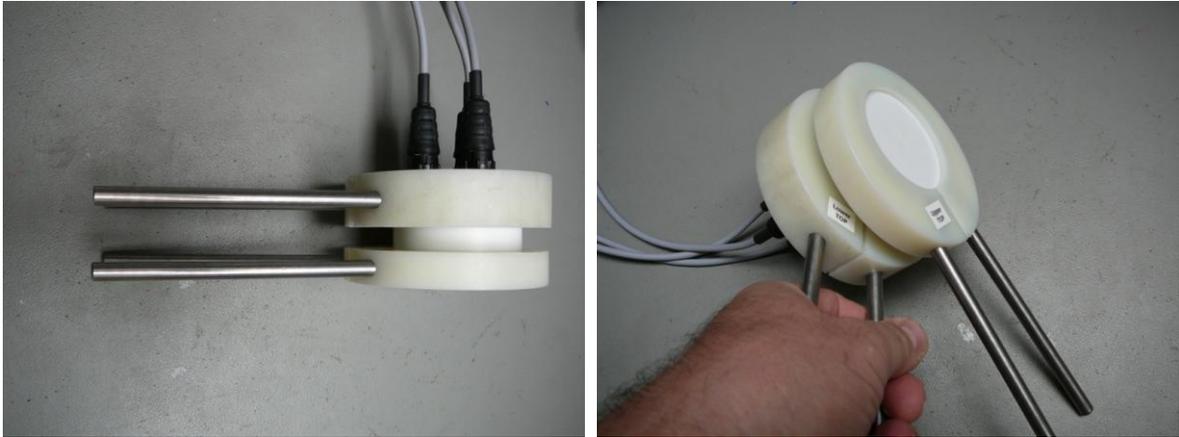

Note 1: Screw back the lid by hand only. Use the tool only for finalizing but with a limited power only!

Note 2: When replacing the battery, short circuit the battery terminals before inserting the new one. Watch polarity. Replace the desiccant bag. Do not forget to initialize the system after the battery replacement.